



Main Trigger Station 2017/03/28 更新

LLA	LOGIC LEVEL ADAPTER
2NTF	2CH NIM/TTL FANOUT
6TF	6ch TTL FANOUT
GDG	2CH GATE & DELAY GENERATOR
24PA	24V PULSE AMP
8LLF	8CH LOGIC LEVEL FANIN/FANOUT
50Hz	2CH 50Hz MONITOR
AND	NIM LOGIC AND/FANOUT
TLC	TRIGGER LEVEL CONVERTER 24V→5V TRIG I

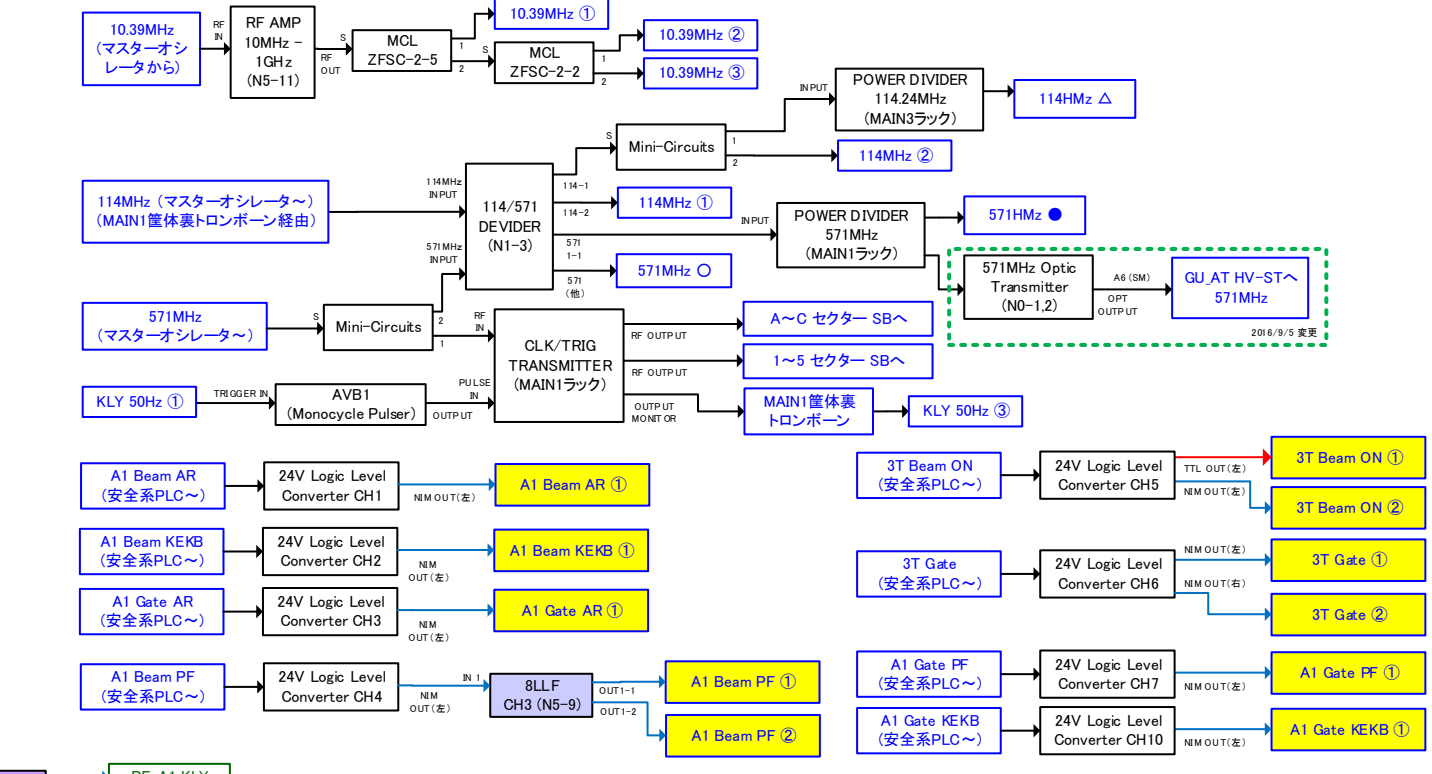

TD4V撤去への変更箇所
TRIPLE SYNC 導入への変更箇所

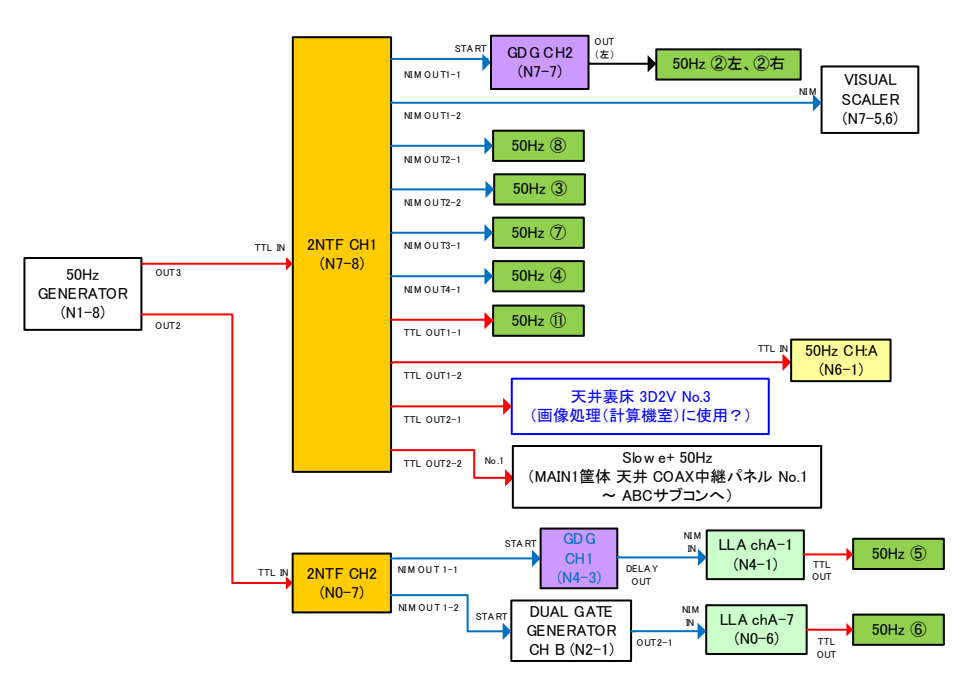